

Licel PM-HV

Photomultiplier Module

Manual

April 22, 2009

Contents

1	Product description	3
2	Handling of PMTs	3
3	Operation of PMTs	3
4	Pulse Height Distribution	4
5	Using the PMT in a LIDAR	7
5.1	Maximum DC Signal	7
5.2	Peak Signal	7
5.3	Cathode structure	7
5.4	Analog Measurements	7
5.5	Analog and Photon counting	7
5.5.1	Analog Detection	8
5.5.2	Photon counting	8
5.5.3	Paralyzable System	9
5.5.4	Nonparalyzable System	9
5.6	Typical Dead Time Values	9
5.7	Discriminator threshold and dead time values	9
6	Mechanical Dimensions	10
7	High Voltage Control Pinout	11
7.1	H11 connector on the rear side of the PMT-HV cassette	11
8	Specifications	12

1 Product description

The High Dynamic Range Photomultiplier from Licel has been specifically optimized to enhance the results of your measurements in pulsed applications. The compact design combines a stabilized dynode chain for strong light pulses with fast rise times and narrow pulse widths for high single photon count rates. This combination allows high dynamic range measurements by using both analog and photon counting measurements together, thus extending the linear dynamic range to 5 orders of magnitude.

Additional advantages are reduced space charge effects and higher light levels that can be measured without suffering from nonlinearities. These qualities make the Licel High Dynamic Range Photomultiplier your ideal detector for applications such as Lidar, fluorescence detection and other spectroscopic methods

2 Handling of PMTs

It is recommended that photomultipliers are stored in the dark and are protected from excessive light also during installation. After illumination the dark current will be temporarily increased. Especially the red sensitive cathode type R7400-20 is sensitive and should be kept in dark also during the mounting procedure.

Do not store or use photomultipliers in a helium rich atmosphere. Helium will diffuse through the housing and destroy the internal vacuum.

3 Operation of PMTs


High voltages used in photomultipliers may present a shock hazard. The combination of high voltage and large capacitors can be fatal. When operating PMTs always make sure that the housing of both PMT and HV supply are properly grounded.

The high voltage setting must be in compliance with the average maximum anode current (100uA over 30 seconds for all R7400 PMT's). The max. cathode voltage of 1000V should not be applied for more than 30 seconds. Continuous high voltage settings should not exceed 950V.

When the max. allowed anode average current is exceeded, one dynode is temporarily turned off to prevent damage to the last dynodes. The switching will occur after 10-20 seconds after the 100uA limit is exceeded by 10% and will occur faster if the limit is exceeded further. See the figure in the attached document for the typical switching characteristics. The activation of this protection circuit should be avoided. Data acquired with an activated protection circuit are not meaningful because the

PMT gain will fluctuate when the protection is turned on and off consecutively.

Max. continuous output signal: -6mV

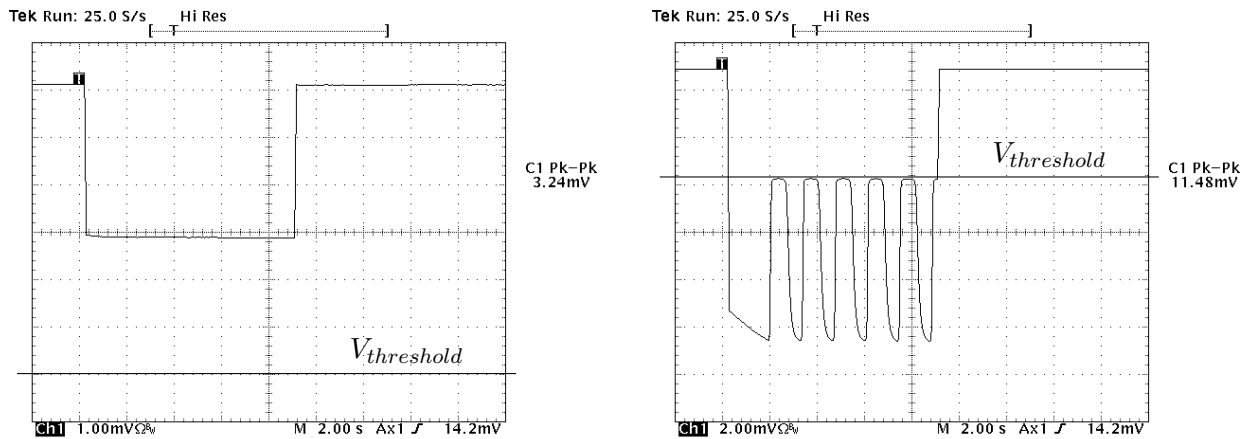

The high voltage setting should be set according to your signal strength and signal shape. If your peak signal amplitude is always below 20mV (into 50 Ω) the recommended HV setting is 850V.

If your peak signal amplitude is higher, reduce the high voltage until the max. amplitude is not above 100mV for more than 50us or not above 500mV for more than 10 us. The specified gain reduction of 10E-3 is achieved when using high voltage settings between 750V and 850V.

4 Pulse Height Distribution

When operating a PMT in photon counting mode the question is: Where to put the discriminator level? From the signal to noise ratio point of view the optimum will be a level where most of the noise counts are removed while only a minor part of the signal is lost. This point is called the valley point.

The pulse height distribution can be shown using two modes:

Integral Mode: All counts below the specified the discriminator level are shown.


Differential Mode: Here the counts with a pulse height between the current and the adjacent discriminator level are shown.

In order to acquire a pulse height distribution set the PMT to a desired voltage and illuminate the PMT using a continuous light level. We have found, that a signal with a mean count rate of 2 MHz or 0.1 count per 50 nsec bin is just fine. A sky with scattered clouds is definitely not stable enough. A LED powered by a DC supply is preferred.

So before running the PHD software the corresponding light levels should be set up. As reference level we use a discriminator level of 10, which corresponds to 3mV. A typical dark PMT will show only few counts or none at all after 1000 shots.

When the continuous light is applied the signal rises to 0.1 count per bin or 2MHz count rate at


discriminator level 8 (-2.5mV).

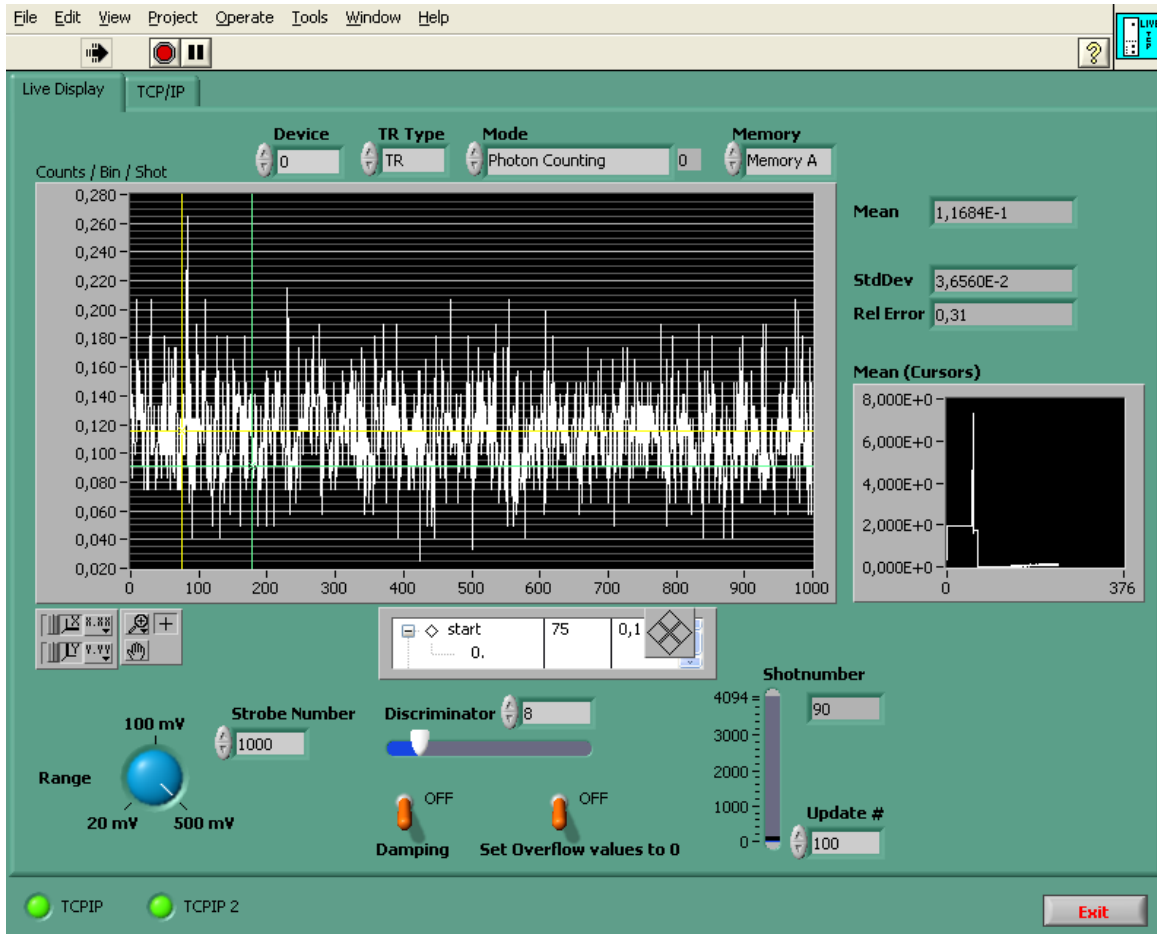

Use the TCP/IP Pulse Height Distribution.vi from the TCP/IP-Pulse.llb or the TCP/IP Pulse Height Distribution.exe if you prefer the executable.

The first step is to press the LabView typical Run button.

You should then select the transient recorder at the Device control and the transient recorder type (TR-xx-xx or PR-xx-xx)

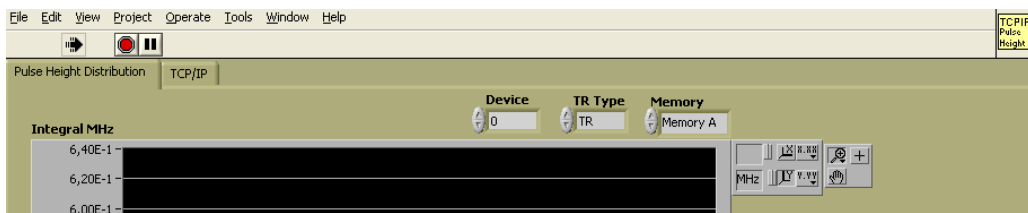


While a shot number of 100 shots per discriminator level is fine for an integral pulse height distribution, you should select significantly more for a differential pulse height, for instance 4000 shots. Acquire 4000 * 63 shots to get the PHD. A typical pulse height measurement using a 30Hz laser as the trigger source would require 2.3h of total acquisition time. The TR 20-160 can run at 300Hz, which will cut the acquisition time down to 840 sec or 14min. Using a faster trigger source is therefore recommended.

The illumination level must be kept constant over this period of time as it would otherwise distort the the PHD.

A typical sample of a integral PHD with 100 shots per discriminator level is shown below. Press the Start button to begin the data acquisition. The data display will be updated once the shots for a


discriminator level are acquired.

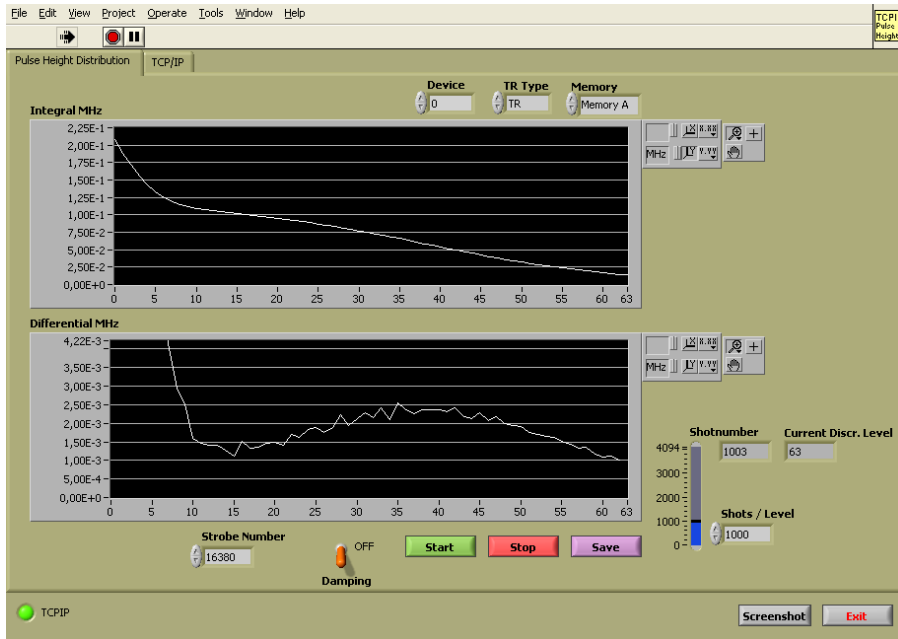

Please notice the change in the slope around discriminator level 10. The differential PHD for the same light intensity makes that more obvious. Select the differential field on the right side of the data display to get the differential PHD.

Here the valley point can be seen at discriminator level 10 which should then be used in the acquisition program. As the valley is not very sharp a discriminator level of 8 might also be a good choice.

These values can then be used in the configuration data of the transient recorder in the acquisition program.

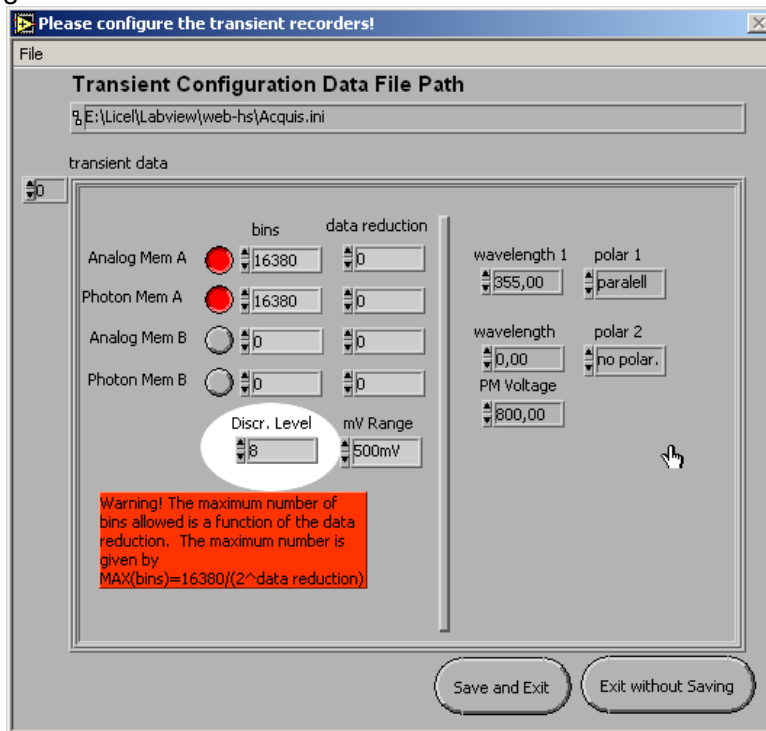

5 Using the PMT in a LIDAR

5.1 Maximum DC Signal

The maximum allowed average anode current for a R7400 PMT is 100 μA . This corresponds to 5mV in the analog mode at a 50 Ω input. **This should never be exceeded.** The Licel PMT has a high current clamp down which will reduce the signal once more than 120 μA are drawn from the tube for more than 100...1000ms. If this happens the signal will be severely distorted and not useful for any LIDAR measurement. 5mV background signal can be easily reached during day time when the field stop is not small enough or the interference filters are too wide. Reducing the high voltage below 800V might help on first glance but is not optimal as a long term solution. The PMT cathode can provide a limited amount of photons over its lifetime, exposing the tube to a constant DC light will shorten this lifetime.

5.2 Peak Signal

The peak signal can significantly exceed the background level as long as the integral current is below 100 μA . The analog signal should fit into the input range of the preamplifier and the ADC. Due to the fluctuations of the lidar signal the following rule of thumb will keep the signal inside the ADC range.

The peak signal should not exceed half of the input range.

For a 100mV input range this corresponds to 50mV.

5.3 Cathode structure

The cathode of the PMT has an inhomogenous sensitivity due to the dynode structure which will result in signal modulations if the signal spot changes its position on the cathode between then near and the far field signal. To avoid this the primary mirror should be imaged on the detector rather than the field stop.

5.4 Analog Measurements


For analog measurements a background profile is mandatory as otherwise ADC slopes or electromagnetic interference will be taken as real atmosphere response.

5.5 Analog and Photon counting


The Licel transient recorder systems have a parallel analog and photon counting detection chain. The combination of both signals allows using the high linearity of the analog signal for strong signals and the high sensitivity of the photon counting for weak optical signals. The integration of both detection mechanism into a single device avoids ground loops and other problems that make the combination otherwise cumbersome. The main idea of the signal combination is that there is a region where both signals are valid and have a high signal to noise ratio. For typical Mini-PMT this region extends from 0.5 to 10 MHz in the photon counting.

To combine (glue) both signals, the photon counting needs a dead time correction.

5.5.1 Analog Detection

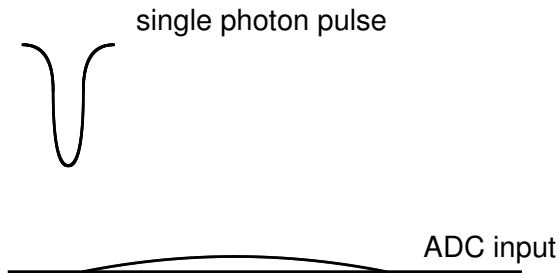


The single pulse from the PMT is passed through a anti-alias filter and then preamplified. The resulting signal is fed into an ADC. For a single pulse only a few ADC bits are used and the noise of the preamplifier and the ADC is comparable to the signal fed into the ADC. Under these conditions photon counting has a higher SNR.

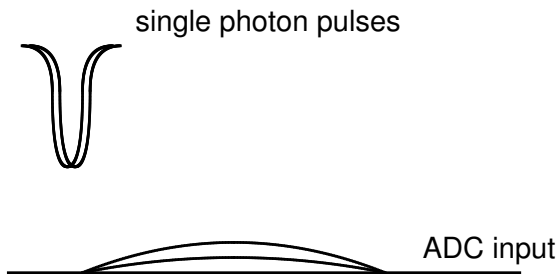

If two single pulses overlap the signal at the ADC will increase proportional. Due to this effect the ADC does not have a dead time constraint even for high count rates. For high count rates the linearity of the analog signal is superior to the photon counting.

5.5.2 Photon counting

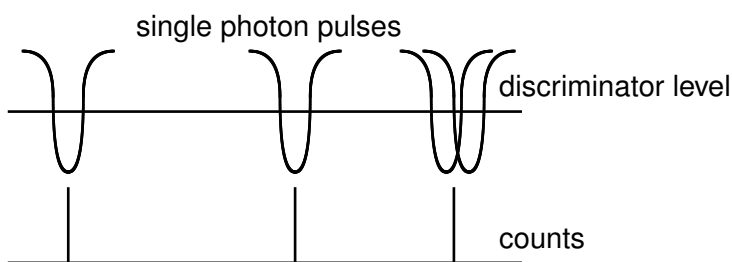

Each single photon pulse is compared to a discriminator threshold. Signals that exceed the threshold cause a count. This is less sensitive to noise and baseline drifts. However due to the statistical nature of the pulses two of them may be so close together that they are not distinguishable at the discriminator and cause only a single count instead of two counts. This is described as the dead-time due to pulse pile up. As a consequence the observed count rate is less than the true incident count rate.

There are two typical dead-time scenarios, while the Licel photon counter can be best described as nonparalyzable. For a detailed discussion of the theory of photon counting dead time correction please see the excellent paper: *D. P. Donovan, J. A. Whiteway, and A. I. Carswell, "Correction for nonlinear photon-counting effects in lidar systems," Appl. Opt. 32, 6742-6753 (1993).*

5.5.3 Paralyzable System

For a paralyzable system a single photon starts a dead time which can be extended by the next photon that arrives within the dead-time. For instance photon are 4ns wide and one photon follows 2ns and 5ns after the first one, the count will be 1 as the dead time starts again with the second photon.

$$N = S \exp(-S\tau_d) \quad (1)$$

Where:

- N - is the observed count rate
- S - is the true count rate
- τ_d - is the system dead time

5.5.4 Nonparalyzable System

For a a paralyzable system a single photon starts a dead-time which will not be extended by the next photon that arrives within the dead-time. For instance photon are 4ns wide and one photon follows 2ns and 5ns after the first one, the count will be 2 as the second photon will be suppressed.

$$N = \frac{S}{1 + S * \tau_d} \quad (2)$$

- N - is the observed count rate
- S - is the true countries
- τ_d - is the system dead time

While the paralyzable case is nonlinear equation, the nonparalyzable case can be easily inverted to

$$S = \frac{N}{1 - N * \tau_d} \quad (3)$$

As both cases are only a theoretical model, they are valid for lower count rates but fail when $S * \tau_d$ becomes larger than one. From a numerical point of view Eq. 3 can be only applied to a signal as long as

$$N < \tau_d \quad (4)$$

As an example the correction factor for a time constant of 4ns and a observed count rate of 5 MHz is 1.02. As typical averaged maximum observed count rate is 160MHz the correction factor would be 2.77. This would imply an maximum count rate of 470MHz. The glued profiles however show a virtual count rate in the 2GHz region for a 20mV peak.

5.6 Typical Dead Time Values

The observed dead times are always a combination of different dead times. The detector pulse width, as the discriminator level and the dead time of the photon counter itself influence the values. For the nominal values for the HV (850V) and a discriminator level of 8 at the Licel transient recorder (which is a good starting point for photon counting lidar setup) we found that 3.7ns or 270MHz is a good estimate.

5.7 Discriminator threshold and dead time values

When the discriminator threshold is lowered the observed count rate increases. There are two physical limits that work against this, if the threshold is very low, level 0 till 2 one will loose the advantages

of photon counting and become vulnerable to electromagnetic noise. In extreme cases a continuous counting can be observed where the signal appears as inverted as the pulses corresponding to photons will elevate the voltage level over the electromagnetic noise and the observed count rate will drop.


For low discriminator levels it is possible that the same photon pulse is counted twice once as the normal peak and once for the ringing after the peak. The signal will be partly proportional to the incident light flux, however nonlinearities should be expected that are difficult to correct for. A typical test is to verify that a constant low light level produces counts that adhere to the Poisson statistic.

On the opposite side rising the discriminator level, will throw away a significant part of the small photons and reduce the observed dead time. The highest linear range will be achieved when half of all photon pulses are thrown away. This linearity comes at a high price, the dead time correction models do not work anymore and the system becomes more fragile as small changes in the discriminator and high voltage of the PMT will significantly influence the result. The method is known in the literature as a physical dead time correction.

A related issue is a hyper linear behavior if the discriminator threshold leads to large portions of the small counts to be thrown away. For low count rates this does not negatively influence the signal. However for medium strong signals the following will happen: two small photons that would be normally discriminated will form a countable photon if they overlap. They might compensate the loss in count rates for larger photons that overlap. This is the mechanism that is described above. However if they overcompensate, the observed count rate will exceed what should be a linear response. A typical observation of this behavior is that for glued profiles the pure photon counting exceeds the glued count rate over the gluing point.

A pulse height distribution where the pulses are all small and no valley point can be observed can lead to this behavior. If such a pulse height distribution is observed, there are two recommendations, first increase the high voltage, this will make the photons larger, second decrease the discriminator level. However the limitations that are outlined above also apply in this case.

6 Mechanical Dimensions

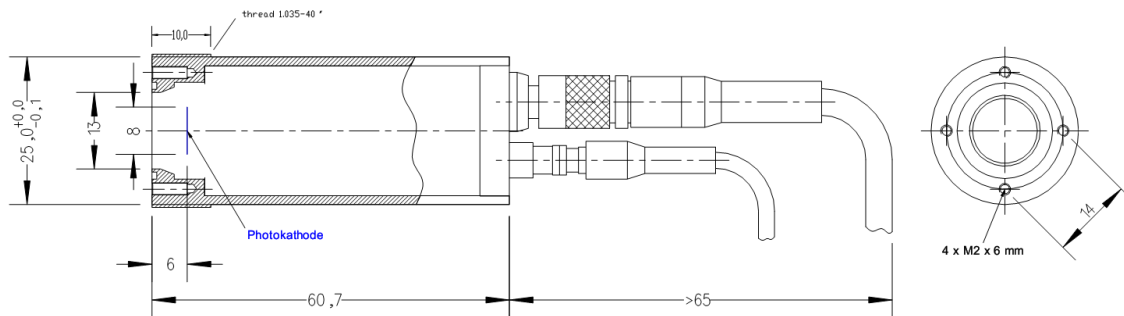

all dimensions in mm

7 High Voltage Control Pinout

7.1 H11 connector on the rear side of the PMT-HV cassette

Pin	Description
2	+13...+15V in (max. 280mA)
5	Gnd
8	+5V Reference out
11	Gnd
14	Inhibit (high = off)
17	+12V Reference out
20	Gnd
23	Remote HV Control, 0..+1V into 100kOhm
26	Voltage Monitor (-5mV/V)
29	Current Monitor (2mA/V)
32	Protective Gnd (Case)

8 Specifications

Detector:

cathode diameter:	8 mm
spectral sensitivity	
Bialkali cathode-06:	160-650 nm
Bialkali cathode-03:	185-650 nm
Multialkali cathode-01:	300-850 nm
Multialkali cathode-02:	300-880nm
Multialkali cathode-20:	300-900nm
Multialkali cathode-04:	185-850 nm
max. average anode current:	0.1 mA
gain:	10^5 - 10^6

Signal specs:

single photon rise time:	<1.3 ns
single photon width (FWHM):	<2.2 ns
pulse load stability, HV=850V, 100mV signal / 60 μ s	<0.15%

HV supply:

voltage range:	-100...-1kV
max. current:	2 mA
voltage ripple:	<1 mV (DC to 20 MHz)
remote control voltage:	0..+1V
Mechanics:	
PMT module size:	60.7 x 25mm
PMT module weight:	50 g
Optical interface:	O-ring sealed mount or adapter for 1" Thorlabs lens tube system
High voltage supply:	50.5x128.4x103mm 3 height units, 10 width units standard cassette

Connectors:

Signal out:	Minax/BNC 2m
HV to PMT:	Lemo Camac 2m
HV power supply:	H11 connector
Power supply:	15V DC, 250mA

Environmental conditions:

Operating temperature:	0°C to 30°C (non condensing)
Storage temperature:	-40°C to 70°C

System integration:

Mating parts of Thorlabs Lens tube system SM1L03, SM1L05,...1" stackable lens tubes
SM1NT Locking Nut and other components of the SM1 series